



## RPA Exo Kit

✉ [info@ezassay.com](mailto:info@ezassay.com)

🌐 [www.ezassay.com](http://www.ezassay.com)

EZassay Biotechnology Ltd.

Catalog Code: EX-LYO-48  
EX-LYO-96

# CONTENTS

<u>Contents</u>	<u>Page</u>
Brief introduction	1
Materials supplied	1
Required materials but not supplied	1
Storage	1
Assay procedure	2
Notes	3
Schematic diagram of working principle of Exo kit	4
Design principles of probe for Exo kit	4
Choose the right product	5

## Brief introduction

This kit provides the essential components required for recombinase polymerase amplification (RPA) of nucleic acids. It offers high sensitivity, strong specificity, and rapid amplification.

The reaction is performed at a constant temperature of 37–42 °C, with amplification typically completed within 30 minutes.

The assay features a simple workflow, minimal equipment requirements, and can be carried out under isothermal conditions, making it well suited for POCT assay and product development.

## Materials supplied

Item	EX-LYO-48	EX-LYO-96
RPA Reaction Tubes	48T	96T
Rehydration Buffer (2X)	500µL	500µL*2
Positive control (10X)	10µL	10µL*2
Starter (10X)	100µL	100µL*2

## Required materials but not supplied

1. RPA primers and probe (online software: <https://www.ezassay.com/primer>)
2. Fluorescent reader such as qPCR thermocycler
3. Nuclease-free water
4. DNA template

## Storage

-20°C

## Assay procedure


1. Set the qPCR working temperature at 39 °C. (Optimization range 37~42°C)  
(Turn off the lid heating function or set to 42 °C.)
2. For each reaction tube, add reagents as described in the table below. It is recommended to set up the reactions on ice. To minimize pipetting variation, prepare a master mix according to the total number of reactions.

Component	Sample group	Positive control group	Negative control group
Rehydration Buffer(2x)	10μL	10μL	10μL
Forward Primer (20μM)	0.42μL	-	0.42μL
Reverse Primer (20μM)	0.42μL	-	0.42μL
Exo probe (4μM)	0.6μL	-	0.6μL
DNA template	x μL	-	-
Positive control (10X)*	-	2μL	-
Nuclease-free H2O		Up to 18μL	

\* The Positive Control contains primers, the Exo probe, and the DNA template. The probe is labeled with FAM-BHQ1.

3. Add 2 μL of Starter to each RPA Reaction Tube. It is recommended to dispense the Starter onto the inner side of the tube cap or the tube wall.
4. Invert and flick the reaction tube, then briefly centrifuge. Repeat 3 times to ensure thorough mixing. The lyophilized pellet in the RPA Reaction Tube should be completely dissolved and evenly mixed. Avoid vigorous vortexing.
5. Place the RPA Reaction Tube into a qPCR instrument. The reaction typically takes 20–40 minutes.

## EZassay™ RT-RPA Kits improvement and upgrade:

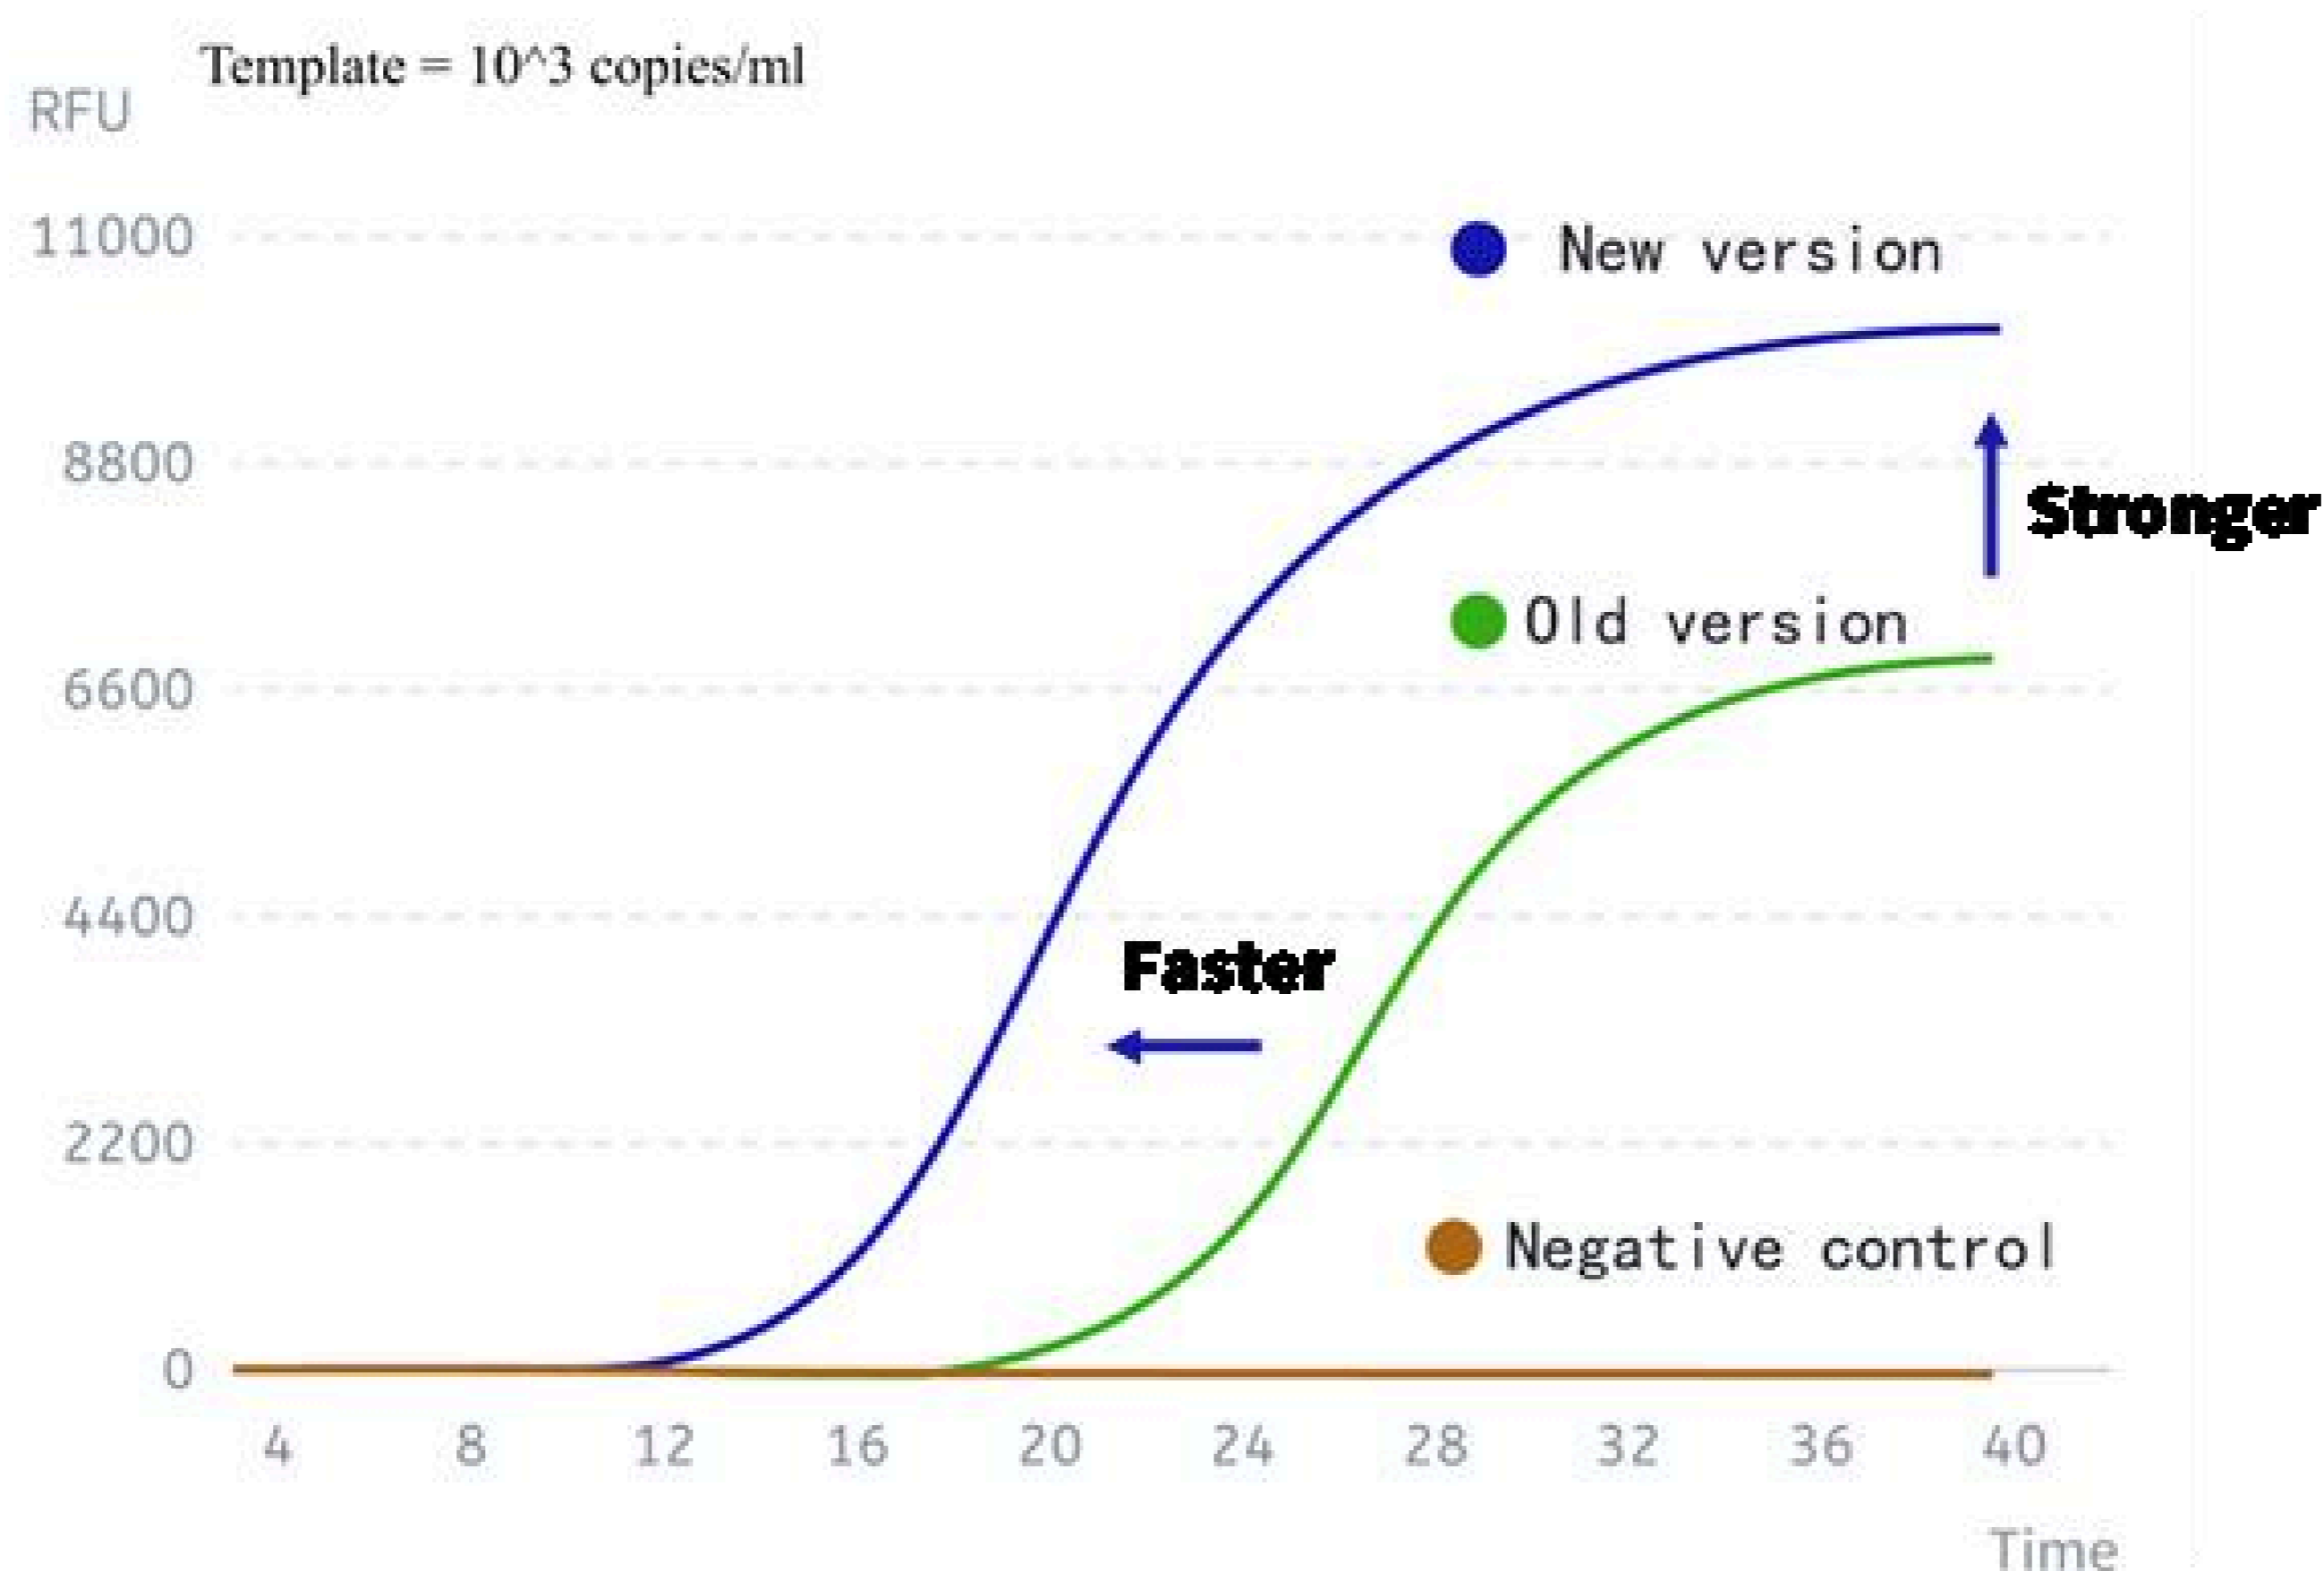

## Notes

- It is recommended to implement physical separation between pre-amplification and post-amplification areas. Independent workspaces, equipment, and consumables should be used for sample preparation, reaction setup, and amplification procedures to minimize the risk of amplicon contamination.

For endpoint detection, ensure that the negative control (NTC) is handled prior to positive samples, and keep the negative control tubes tightly closed when opening positive sample tubes.

If amplicon contamination is suspected, discard the used reagents and replace them with fresh reagent components.

- For samples with low template concentrations, the reaction tube may be gently flicked several times and briefly centrifuged at the 4-minute time point to improve mixing (avoid vigorous shaking), then returned to the original position to continue the reaction.

- Please note that there may be differences between the set temperature and the actual reaction temperature. For first-time use, it is recommended to perform a temperature gradient test, for example by setting up three reactions at 37°C, 39°C, and 41°C to determine the optimal reaction temperature.

- If qPCR instrument is used, please make sure to turn off the heat lid function or set it to 45 °C. For some types, the lid temperature goes up to 105°C immediately after power on. The lid is already hot enough to inactivate enzymes. Please run a few cycles to allow the temperature going down.

- Template recommendations

- Human genomic DNA range for detection is from 1 ng to 500 ng per 20 µL reaction, although 0.1 ng sensitivity can be achieved.

- Bacteria genomic DNA range for detection is from 0.01 ng to 10 ng per 20 µL reaction, although 0.1 pg sensitivity can be achieved.

- Viral DNA/RNA range for detection is from 100 copies per 20 µL reaction, although 1-5 copy sensitivity can be achieved.



5. The distance between the fluorophore and the quencher group should be  $\leq 5$ nt;
6. The distance between the fluorophore and THF site, the quencher group and THF site should be between 0~2nt, and the maximum should not exceed 2nt, otherwise the cleavage effect of Exonuclease will be poor;
7. When using FAM as the fluorophore, it is recommended to use BHQ1 as the quencher, and BHQ2 as the quenching group when using TAMRA as the fluorophore.
8. The concentration of the probe can be optimized between 50 nM and 150 nM;
9. The primer design of Exo kit is the same as basic kit. The probe design can be carried out after primer screening. Probe should be between the upstream and downstream primers. Over-lap can be accepted.
10. Fluorescence reader is needed to interpret the results, such as a thermostatic amplification instrument with fluorescence collection or ABI-7500, Roche 480 and other qPCR instruments;
11. Please note that amplicons will generally be cut by Exonuclease. There is no clear band when you run DNA gel.

## Choose the right product

Product name	Classify	Template	Catalog number	Brief introduction
RPA/RAA Isothermal amplification	Basic kit	DNA	BA-LYO-96	Similar to PCR, it is mainly used to complete DNA amplification. You can observe the results with DNA gel. You can also combine it with CRISPR technology.
		RNA	BA-RT-LYO-96	
	Exo kit	DNA	EX-LYO-96	Based on the basic kit, a fluorescent probe (Exo probe) is introduced. It is similar to fluorescent probe PCR. Fluorescent signals can be read with a fluorometer.
		RNA	EX-RT-LYO-96	
	Nfo kit	DNA	NF-LYO-96	Based on the basic type, lateral flow probe (Nfo probe) is introduced. Test results can be observed with lateral flow paper strips.
		RNA	NF-RT-LYO-96	